

Certificate of Analysis SALSA® MLPA® Probemix P093 HHT/HPAH

| Catalogue # | P093-025R, P093-050R, P093-100R | |
|-----------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------|
| Product name | Probemix P093 HHT/HPAH | |
| LOT | C2-1122 | |
| Σ | 25, 50, or 100 reactions. | |
| Shipping conditions | Dry ice or cooling elements. | |
| X | Store upon arrival between -25°C and -15°C. | |
| | Expiration date: November 2027, when stored at recommended conditions. This product should not be frozen/thawed more than 25 times. | |
| Purpose | This product has been developed to determine the DNA copy number of the human <i>ENG</i> , <i>ACVRL1</i> and <i>BMPR2</i> genes, as described in table 1 and 2 of the product description. This probemix is designed for use only in combination with SALSA MLPA reagent kits and Coffalyser.Net analysis software as described in the MLPA General Protocol. | |
| Quality control specifications | Sufficient distance between peaks, absence of extra or shoulder peaks, and completeness of hybridisation of each individual probe, as tested on Applied Biosystems and Beckman/SCIEX GeXP sequencers. Standard deviation of each individual probe ≤0.10, when tested on 23 different DNA samples of healthy individuals, extracted by various methods. | Test result |
| | Each individual probe meets reaction-specific criteria when tested on a single DNA sample under various experimental conditions. No-DNA controls result in only five major peaks shorter than 121 nucleotides (nt): four Q-fragments at 64, 70, 76 and 82 nt, and one peak in the range of 0-40 nt corresponding to the unused portion of the fluorescent PCR primer. Non-specific peaks longer than 121 nt AND with a height <25% of the median of the four Q-fragments are not expected to affect MLPA reactions when sufficient (50-250 ng) sample DNA is used. Note: We observed one prominent peak below the 25% threshold with a length of approximately 178 nt in a No-DNA control | PASS |

None of the ingredients are derived from humans, animals, or pathogenic bacteria. Based on the concentrations present, none of the ingredients are hazardous as defined by the Hazard Communication Standard. **A Safety Data Sheet (SDS) is not required for these products**: none of the preparations contain dangerous substances (as per Regulation (EC) No 1272/2008 [EU-GHS/CLP] and amendments) at concentrations requiring distribution of an SDS (as per Regulation (EC) No 1272/2008 [EU-GHS/CLP] and 1907/2006 [REACH] and amendments). If spills occur, clean with water and follow appropriate site procedures.

| More information: www.mrcholland.com; www.mrcholland.eu | | |
|---------------------------------------------------------|------------------------------------------------------------------------------------------|--|
| *** | MRC Holland bv; Willem Schoutenstraat 1 1057 DL, Amsterdam, The Netherlands | |
| E-mail | info@mrcholland.com (information & technical questions) order@mrcholland.com (orders) | |
| Phone | +31 888 657 200 | |



Certificate of Analysis SALSA MLPA Probemix P093-C2 HHT/HPAH sample picture

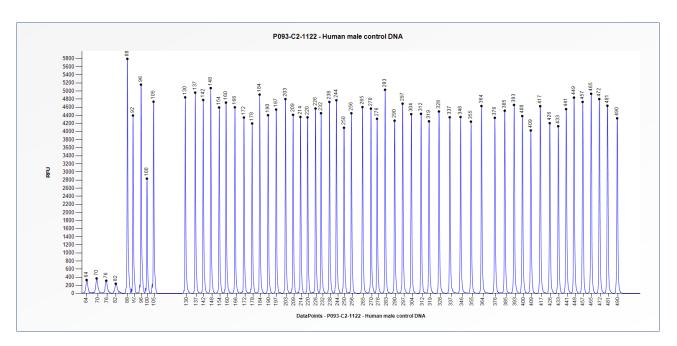


Figure 1. Capillary electrophoresis pattern from a sample of approximately 50 ng human male control DNA analysed with SALSA MLPA Probemix P093 HHT/HPAH (C2-1122).

This lot was certified by MRC Holland on 02 May 2023.

This certificate is a declaration of analysis at the time of the manufacturing process. All assays were run in compliance with manufacturer's instructions for use.

Implemented changes in the COA

Version 01 – 02 May 2023 (6) - Not applicable, new document.